
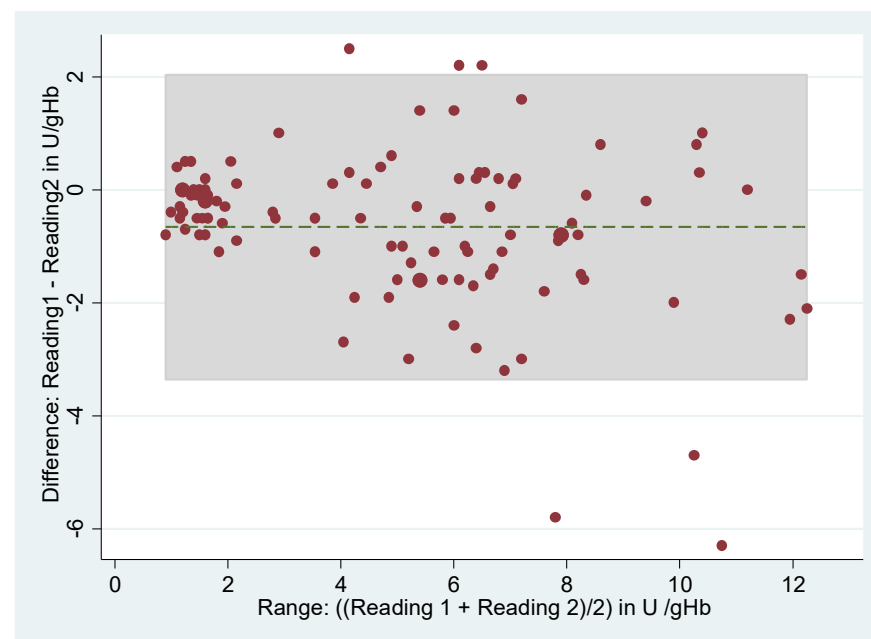


Supp. Figure 2: Repeatability of two measurements of the STANDARD™ G6PD in the field- a) Scatter plot and b) Bland – Altman plot

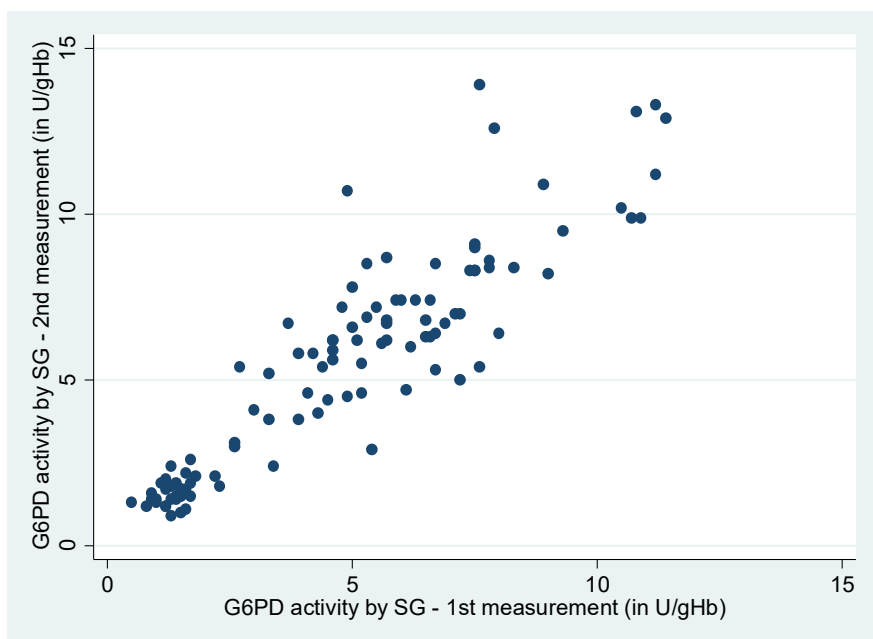

a) $r_s=0.9025$; $p<0.001$, $n=106$ b) Mean difference:- 0.66 U/gHb, 95% LoA: -2.04 to 3.36 U/gHb (grey shaded area)