
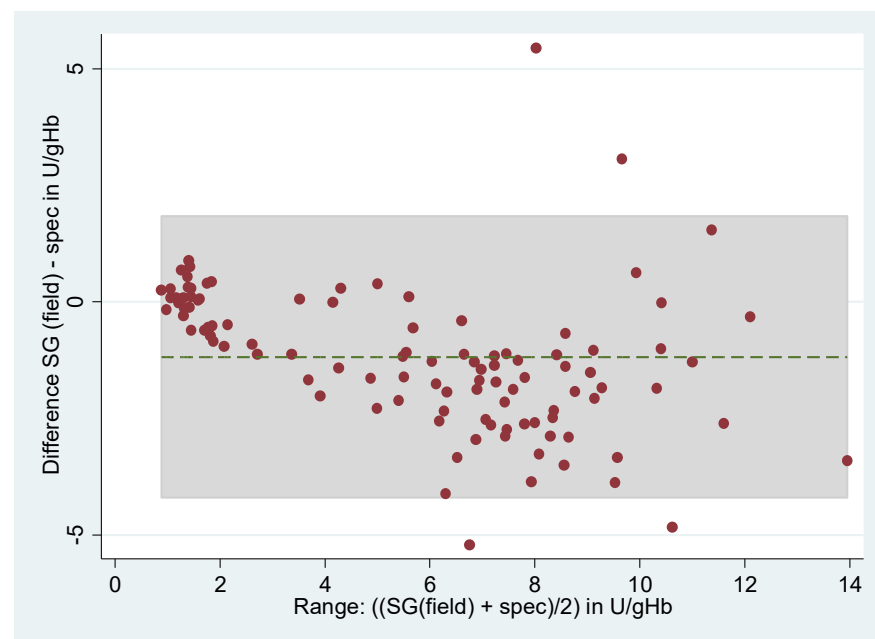


Supp. Figure 4: Comparison of the STANDARD™ G6PD Test (SG) in the field against spectrophotometry a) Scatter plot and b) Bland-Altman plot

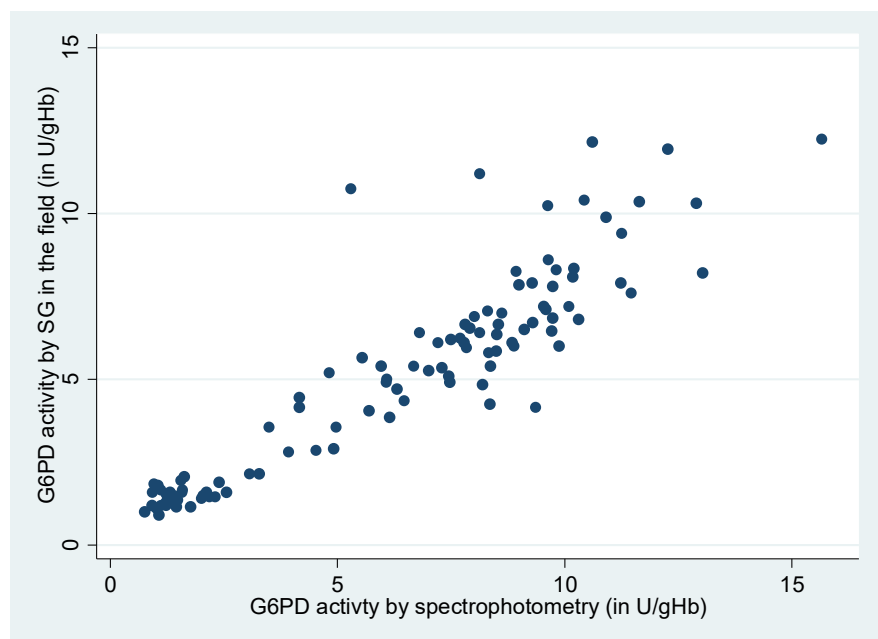

a) $r_s=0.9122$; $p<0.001$, $n=106$ b) Mean difference: -1.18 U/gHb, 95% LoA: -4.20 to 1.84 U/gHb (grey shaded area)